



## CheKine™ Micro Plant Oligomeric Proantho Cyanidins (OPC) Assay Kit

Cat #: KTB1520

Size: 48 T/48 S    96 T/96 S

	<b>Micro Plant Oligomeric Proantho Cyanidins (OPC) Assay Kit</b>		
<b>REF</b>	<b>Cat #:</b> KTB1520	<b>LOT</b>	<b>Lot #:</b> Refer to product label
	<b>Detection range:</b> 0.39-50.00 mg/g		<b>Sensitivity:</b> 0.39 mg/g
	<b>Applicable samples:</b> Plant Tissues		
	<b>Storage:</b> Stored at 4°C for 6 months, protected from light		

### Assay Principle

Oligomeric Proantho Cyanidins (OPC) are a class of polyphenolic compounds of flavanol monomers and their polymers. They are widely present in various organs of plants. They have strong antioxidant and free radical scavenging effects. Used in medicine, food, cosmetics, health care products industry. CheKine™ Micro Plant Oligomeric Proantho Cyanidins (OPC) Assay Kit provides a simple method for detecting OPC concentration in a variety of biological samples such as plant tissues. Under acidic conditions, the resorcinol and phloroglucinol on the A ring of plant proanthocyanidins undergo condensation reaction with vanillin to produce colored compounds. There is a characteristic absorption peak at 500 nm. The light absorption value at 500 nm can be measured to calculate the procyanidins content. The kit is used for testing plant samples.

### Materials Supplied and Storage Conditions

Kit components	Size		Storage conditions
	48 T	96 T	
Extraction Buffer	70 mL	70 mL×2	4°C
Hydrochloric Acid	12 mL	24 mL	4°C
Vanillin	Powder×1 vial	Powder×1 vial	4°C, protected from light
OPC Standard	Powder×1 vial (5 mg)	Powder×1 vial (5 mg)	4°C, protected from light

**Note:** Before formal testing, it is recommended to select 2-3 samples with large expected differences for pre-experiment.

### Materials Required but Not Supplied

- Microplate reader or visible spectrophotometer capable of measuring absorbance at 500 nm
- 96-well plate or microglass cuvette, precision pipettes, disposable pipette tips
- Centrifuge, ice maker, 40 mesh sieve
- Deionized water, methanol
- Homogenizer, Ultrasonic disruptor

## Reagent Preparation

**Extraction Buffer:** Ready to use as supplied. Equilibrate to room temperature before use. Store at 4°C.

**Hydrochloric Acid:** Ready to use as supplied. Equilibrate to room temperature before use. Store at 4°C.

**Note: Extraction Buffer or Hydrochloric Acid has certain irritation, so personal protection is recommended during use.**

**Vanillin:** Before use, add 6 mL methanol for 48 T, add 12 mL methanol for 96 T. Equilibrate to room temperature before use. Store at 4°C, protected from light for 1 month.

**Working Reagent:** Before use, mix hydrochloric acid and dissolved Vanillin at a ratio of 1:1. Equilibrate to room temperature before use. Working reagent is freshly prepared.

**Blank Working Reagent:** Before use, mix hydrochloric acid and methanol at a ratio of 1:1. Equilibrate to room temperature before use. Blank working reagent is freshly prepared.

**OPC Standard:** Before use, add 1 mL Extraction Buffer to dissolve. The concentration is 5 mg/mL. Equilibrate to room temperature before use. Store at 4°C, protected from light for 2 weeks.

**Setting of standard curve:** Further dilute the 5 mg/mL standard to 2.5, 1.25, 0.625, 0.3125, 0.156, 0.078 and 0 mg/mL standard solution with Extraction Buffer, as shown in the following table.

Num.	Volume of OPC Standard (µL)	Volume of Extraction Buffer (µL)	Standard Concentration (mg/mL)
Std.1	100 µL 5 mg/mL	0	5
Std.2	100 µL of Std.1 (5 mg/mL)	100	2.5
Std.3	100 µL of Std.2 (2.5 mg/mL)	100	1.25
Std.4	100 µL of Std.3 (1.25 mg/mL)	100	0.625
Std.5	100 µL of Std.4 (0.625 mg/mL)	100	0.3125
Std.6	100 µL of Std.5 (0.3125 mg/mL)	100	0.156
Std.7	100 µL of Std.6 (0.156 mg/mL)	100	0.078
Std.8	0	100	0 (Blank Well)

**Note: Always prepare fresh standards per use; Diluted Standard Solution is unstable and must be used within 4 h.**

## Sample Preparation

**Note: Fresh samples are recommended. If not assayed immediately, samples can be stored at -80°C for one month.**

1. Plant tissues with more fibers: the plant tissue can be dried to constant weight, pulverized and sieved by a 40-mesh sieve. Weigh about 0.1 g tissue, add 1 mL Extraction Buffer and mash. Ultrasonic break in ice bath 30 min (power 30% or 300 W, ultrasonic 5 s, interval 8 s). Centrifuge at 12,000 rpm for 10 min at 25°C. Take the supernatant, and dilute the volume to 1 mL with Extraction Buffer, and place it on ice to be tested.

2. Plant tissues with less fibers: Weigh about 0.1 g tissue, add 1 mL Extraction Buffer and mash. Ultrasonic break in ice bath 30 min (power 30% or 300 W, ultrasonic 5 s, interval 8 s). Centrifuge at 12,000 rpm for 10 min at 25°C. Take the supernatant, and dilute the volume to 1 mL with Extraction Buffer, and place it on ice to be tested.

**Note: The Extraction Buffer contains components that denature the protein. If the protein concentration is calculated, the protein needs to be extracted with deionized water for determination.**

## Assay Procedure

1. Preheat the microplate reader or visible spectrophotometer for more than 30 min, and adjust the wavelength to 500 nm, visible spectrophotometer was returned to zero with deionized water.

2. Sample measurement (The following operations are operated in the 96-well plate or microglass cuvette).

Reagent	Standard Well (μL)	Test Well (μL)	Control well (μL)
Sample	0	40	40
Different Concentration of Std.	40	0	0
Blank Working Reagent	0	0	160
Working Reagent	160	160	0

3. Mix well and kept at 30°C for 30 min. The absorbance value is measured at 500 nm. The blank well is marked as  $A_{\text{Blank}}$ , the standard well is marked as  $A_{\text{Standard}}$ , the test well is marked as  $A_{\text{Test}}$ , and the control well is marked as  $A_{\text{Control}}$ . Finally calculate  $\Delta A_{\text{Test}} = A_{\text{Test}} - A_{\text{Control}}$ ,  $\Delta A_{\text{Standard}} = A_{\text{Standard}} - A_{\text{Blank}}$ .

**Note: Blank well and Standard well only need to measure 1 time. In order to guarantee the accuracy of experimental results, it is recommended to do a pre-experiment with 2-3 samples. If the  $\Delta A_{\text{Test}}$  of the sample is greater than 0.6, the sample needs to be appropriately diluted with the Extraction Buffer before measurement. If  $\Delta A_{\text{Test}}$  is less than 0.01, increase the sample quantity appropriately. Note that the dilution factor involved in the calculation formula should be changed accordingly. Colored samples with high anthocyanidin content have relatively greater interference, while OPC are colorless substances.**

## Data Analysis

**Note: We provide you with calculation formulae, including the derivation process and final formula. The two are exactly equal. It is suggested that the concise calculation formula in bold is final formula.**

### 1. Drawing of standard curve

With the concentration of the standard solution as the y-axis and the  $\Delta A_{\text{Standard}}$  as the x-axis, draw the standard curve.

### 2. Calculation of OPC content

Bring the  $\Delta A_{\text{Test}}$  of the sample into the equation to get the y value (mg/mL).

(1) Calculated by fresh weight of samples

$$\text{OPC (mg/g weight)} = y \times V_{\text{Extraction Buffer}} \div W = \mathbf{y \div W}$$


(2) Calculated by protein concentration

$$\text{OPC (mg/mg prot)} = y \times V_{\text{Extraction Buffer}} \div (\text{Cpr} \times V_{\text{Extraction Buffer}}) = \mathbf{y \div \text{Cpr}}$$

Where:  $V_{\text{Extraction Buffer}}$ : Extraction Buffer added, 1 mL; Cpr: sample protein concentration, mg/mL; W: Sample weight, g.

## Typical Data

Typical standard curve:

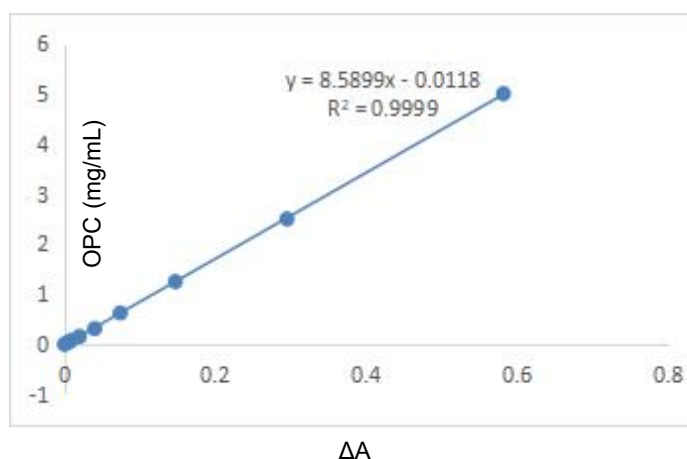

$\Delta A$

3/4

Version 20250530

Figure 1. Standard curve for OPC.

## Recommended Products

Catalog No.	Product Name
KTB1500	CheKine™ Micro Total Antioxidant Capacity (TAC) Assay Kit
KTB1080	CheKine™ Micro Superoxide Anion Scavenging Capacity Assay Kit
KTB1091	CheKine™ Micro Hydroxyl Free Radical Scavenging Capacity Assay Kit
KTB1510	CheKine™ Micro Uric Acid (UA) Assay Kit
KTB1530	CheKine™ Micro Plant Flavonoids Assay Kit
KTB1540	CheKine™ Micro Plant Total Phenols (TP) Assay Kit

## Disclaimer

The reagent is only used in the field of scientific research, not suitable for clinical diagnosis or other purposes. For your safety and health, please wear a lab coat and disposable gloves.