



CheKine™ Micro Reduced Glutathione (GSH) Assay Kit

Cat #: KTB1600

Size: 48 T/48 S 96 T/96 S

	Micro Reduced Glutathione (GSH) Assay Kit		
REF	Cat #: KTB1600	LOT	Lot #: Refer to product label
	Detection range: 2-400 µg/mL		Sensitivity: 2 µg/mL
	Applicable samples: Serum, Plasma, Animal/Plant Tissues, Blood Cells, Cells, Bacteria		
	Storage: Stored at 4°C for 12 months, protected from light		

Assay Principle

Glutathione is a tripeptide of glycine, glutamic acid and cysteine. In the red blood cells, Reduced Glutathione (GSH) is the key to maintain hemoglobin in reduced state and protect cells from oxidative damage. GSH is the most important antioxidant sulfhydryl compound in cells, which plays an important role in oxidation resistance, protein sulfhydryl protection and amino acid transport across membrane. The ratio between reduced and oxidized glutathione (GSH/GSSG) is the main indicator of the cell's redox state. Therefore, measuring the content of GSH and GSSG and the ratio of GSH/GSSG in cells can reflect the redox state of cells. CheKine™ Micro Reduced Glutathione (GSH) Assay Kit provides a simple method for detecting the content of GSH in a variety of biological samples, such as Serum, Plasma, Animal and Plant Tissues, Red Blood cells, Cells, Bacteria. DTNB reacts with reduced glutathione to form a yellow product. The optical density measured at 412 nm, can directly reflect glutathione concentration in the sample.

Materials Supplied and Storage Conditions

Kit components	Size		Storage conditions
	48 T	96 T	
Extraction Buffer	70 mL	70 mL×2	4°C
Assay Buffer	10 mL	20 mL	4°C
Chromogen	4 mL	8 mL	4°C, protected from light
Standard	Powder×1 vial (10 mg)	Powder×2 vials (10 mg)	4°C, protected from light

Note: Before formal testing, it is recommended to select 2-3 samples with large expected differences for pre-experiment.

Materials Required but Not Supplied

- Microplate reader or visible spectrophotometer capable of measuring absorbance at OD412 nm

- Incubator
- 96-well plate or microglass cuvette, precision pipettes, disposable pipette tips
- Refrigerated centrifuge
- Deionized water
- Homogenizer (for tissue samples)

Reagent Preparation

Extraction Buffer: Ready to use as supplied. Equilibrate to room temperature before use. Store at 4°C

Assay Buffer: Ready to use as supplied. Equilibrate to room temperature before use. Store at 4°C

Chromogen: Ready to use as supplied. Store at 4°C, protected from light.

Standard preparation:

Diluted Extraction Buffer: Extraction Buffer was diluted 10 times with deionized water, in a clean plastic tube by diluting 200 µL Extraction Buffer into 1,800 µL deionized water.

10 mg/mL GSH Standard: Prepare 10 mg/mL GSH Standard by dissolve 10 mg Standard with 1 mL deionized water for each tube, 10 mg/mL GSH Standard store aliquots at -20°C for 1 month, protected from light.

Standard curve setting: Using 10 mg/mL GSH Standard, prepare standard curve dilution as described:

Num.	Standard (µL)	Diluted Extraction Buffer (µL)	Concentration (µg/mL)
Std.1	40 µL of 10 mg/mL GSH	960	400
Std.2	100 µL of Std.1 (400 µg/mL)	100	200
Std.3	100 µL of Std.2 (200 µg/mL)	100	100
Std.4	100 µL of Std.3 (100 µg/mL)	100	50
Std.5	100 µL of Std.4 (50 µg/mL)	100	25
Std.6	100 µL of Std.5 (25 µg/mL)	100	12.5
Std.7	100 µL of Std.6 (12.5 µg/mL)	100	6.25

Notes: Always prepare fresh Standards per use; Diluted Std. solution is unstable and must be used within 4 h.

Sample Preparation

Note: Fresh samples are recommended, If not assayed immediately, samples can be stored at -80°C for one month.

1. Animal Tissues: Weigh 0.1 g tissue, add 1 mL Extraction Buffer and homogenize on ice. Centrifuge at 8,000 g for 10 min at 4°C. Use supernatant for assay, and place it on ice to be tested.
2. Plant Tissues: Weigh 0.1 g tissue, add 1 mL Extraction Buffer and mash. Ultrasonic break in ice bath 5 min (power 20% or 200 W, ultrasonic 3 s, interval 7 s, repeat 30 times). Centrifuge at 8,000 g for 10 min at 4°C. Use supernatant for assay, and place it on ice to be tested.
3. Plasma or Serum: Collect plasma or serum using an anticoagulant. Centrifuge at 600 g for 10 min at 4°C. Collect supernatant within 30 min and add equal volume of Extraction Buffer. Centrifuge at 8,000 g for 10 min at 4°C. Use supernatant for assay, and place it on ice to be tested.
4. Blood cells: Collect blood using an anticoagulant. Centrifuge at 600 g for 10 min at 4°C. Discard the upper plasma, then wash the pellet with triple volume of cold PBS 3 times (use PBS resuspend blood cells, centrifuge at 600 g for 10 min at 4°C). Add equal volume of Extraction Buffer, then mix and stand at 4°C for 10 min. Centrifuge at 8,000 g for 10 min at 4°C. Use supernatant for assay, and place it on ice to be tested.
5. Cells or Bacteria: Collect 2×10^6 cells/bacteria for each assay. Wash cells/bacteria with cold PBS twice (resuspend cells/bacteria with PBS, centrifuge at 600 g for 10 min at 4°C). Resuspend in triple volume of cells/bacteria pellet Extraction Buffer,

then ultrasonic break in ice bath 5 min (power 20% or 200 W, ultrasonic 3 s, interval 7 s, repeat 30 times). Centrifuge at 8,000 g for 10 min at 4°C. Use supernatant for assay, and place it on ice to be tested.

Note: The sample extracted by this kit is also suitable for the detection of Glutathione Oxidized (KTB1610). Because the Extraction Buffer contains a protein precipitator, the supernatant cannot be used for protein concentration determination. If the protein content needs to be determined, the same sample needs to be taken and the Extraction Buffer replaced with deionized water for extraction preparation. It will be better to quantify the total protein with Protein Quantification Kit (BCA Assay), Cat #: KTD3001, if the content is calculated by protein concentration.

Assay Procedure

1. Preheat the microplate reader or visible spectrophotometer for more than 30 min, and adjust the wavelength to 412 nm, Visible spectrophotometer was returned to zero with deionized water.
2. Add the following reagents to the 96-well plate or microglass cuvette:

Reagent	Blank Well (μL)	Standard Well (μL)	Test Well (μL)
Sample	0	0	20
Deionized Water	20	0	0
Std.	0	20	0
Assay Buffer	140	140	140
Chromogen	40	40	40

Mix well, Incubate for 2 min at room temperature, protected from light, record the absorbance value at 412 nm as A_{Blank} , A_{Standard} , and A_{Test} . The measured absorbance values of Standard Well and Test Well should minus the absorbance of Blank Well, that is, $\Delta A_{\text{Standard}} = A_{\text{Standard}} - A_{\text{Blank}}$, $\Delta A_{\text{Test}} = A_{\text{Test}} - A_{\text{Blank}}$.

Note: In order to guarantee the accuracy of experimental results, need to do a pre-experiment with 2-3 samples. If the ΔA_{Test} of Samples are higher than the ΔA_{Test} of the 400 μg/mL standard, dilute sample with deionized water and repeat this assay. Multiply the results with the dilution factor: n. If ΔA_{Test} is less than 0.01, the sample size can be increased.

Data Analysis

Note: We provide you with calculation formulae, including the derivation process and final formula. The two are exactly equal. It is suggested that the concise calculation formula in bold is final formula.

1. Drawing the standard curve:

With the concentration of the Standard Solution as the y-axis and the $\Delta A_{\text{Standard}}$ as the x-axis, draw the standard curve. Substitute the ΔA_{Test} into the equation to obtain the y value (μg/mL), The GSH concentration (μg/mL)=y.

2. Calculate the content of GSH in sample

(1) By sample fresh weight

$$\text{GSH } (\mu\text{g/g}) = y \times V_{\text{sample}} \div (V_{\text{sample}} \div V_{\text{Extraction}} \times W) \times n = \mathbf{y \div W \times n}$$

(2) Calculated by protein concentration

$$\text{GSH } (\mu\text{g/mg prot}) = y \times V_{\text{sample}} \div (V_{\text{sample}} \times \text{Cpr}) \times n = \mathbf{y \div \text{Cpr} \times n}$$

(3) Calculated by cells or bacteria number

$$\text{GSH } (\mu\text{g}/10^4) = y \times V_{\text{sample}} \div (V_{\text{sample}} \div V_{\text{Extraction}} \times \text{cells or bacteria number}) \times n = \mathbf{y \div 500 \times n = 0.002 \times y \times n}$$

(4) Calculated by liquid volume

$$\text{GSH } (\mu\text{g/mL}) = \mathbf{y \times 2 \times n}$$

Where: W: sample weight, g; V_{sample} : Sample volume added, 2 μL; $V_{\text{Extraction}}$: Extraction Buffer volume added, 1 mL; n: Dilution factor; Cpr: Supernatant protein concentration, mg/mL; 500: Total number of cells or bacteria, 5×10^6 ; 2: Double the dilution during liquid extraction.

Typical Data

Typical standard curve

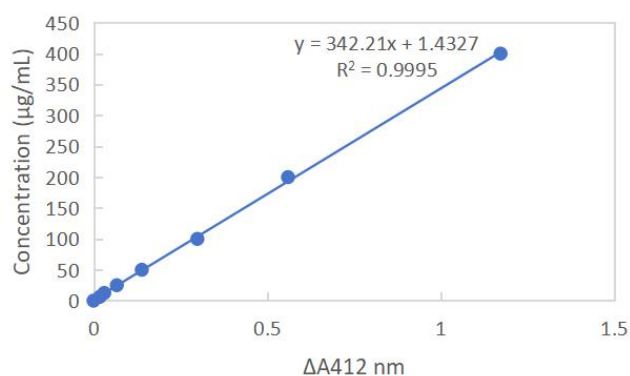


Figure 1. Standard curve of GSH in 96-well plate assay-data provided for demonstration purposes only. A new standard curve must be generated for each assay.

Recommended Products

Catalog No.	Product Name
KTB1610	CheKine™ Micro Glutathione Oxidized (GSSG) Assay Kit
KTB1620	CheKine™ Micro Glutathione Reductases (GR) Assay Kit
KTB1630	CheKine™ Micro Glutathione S-Transferase (GST) Assay Kit
KTB1640	CheKine™ Micro Glutathione Peroxidase (GSH-Px) Assay Kit

Disclaimer

The reagent is only used in the field of scientific research, not suitable for clinical diagnosis or other purposes. For your safety and health, please wear a lab coat and disposable gloves.