



CheKine™ Micro Plant Ammonium Nitrogen Assay Kit

Cat #: KTB3081

Size: 48T/96 T

	Micro Plant Ammonium Nitrogen Assay Kit		
REF	Cat #: KTB3081	LOT	Lot #: Refer to product label
	Applicable sample: Plant sample		
	Storage: Stored at 4°C for 12 months, protected from light		

Assay Principle

Ammonium nitrogen can be directly absorbed and utilized by plants, or converted into nitrate nitrogen by nitrifying microorganisms, and then assimilated into organic nitrogen compounds by plants or microorganisms. Ammonium nitrogen can react with sodium hypochlorite and phenol in strong alkaline medium to produce water-soluble blue dye indophenol blue. The product has a characteristic absorption peak at 625 nm, and the absorbance value is proportional to the content of ammonium nitrogen.

Materials Supplied and Storage Conditions

Kit components	Size		Storage conditions
	48 T	96 T	
Extraction Buffer	55 mL	110 mL	4°C
Reagent I	1	1×2	4°C, protected from light
Reagent II	4 mL	8 mL	4°C, protected from light
Reagent III	1 mL	2 mL	4°C
Standard	1 mL	1 mL	4°C

Materials Required but Not Supplied

- Microplate reader or visible spectrophotometer capable of measuring absorbance at 625 nm
- 96-well plate or microglass cuvette, precision pipettes, disposable pipette tips
- Thermostatic shaker, centrifuge
- Deionized water
- Homogenizer

Reagent Preparation

Extraction Buffer: Ready to use as supplied. Equilibrate to room temperature before use. Store at 4°C.

Reagent I: Prepare before use, add 4 mL deionized water to each tube according to the dosage, and use after fully dissolving. Store at 4°C, protected from light.

Reagent II: Ready to use as supplied. Equilibrate to room temperature before use. Store at 4°C, protected from light.

Reagent III: Ready to use as supplied. Equilibrate to room temperature before use. Store at 4°C.

Standard: Ready to use as supplied. Equilibrate to room temperature before use. Store at 4°C.

Standard preparation: Use 500 µmol/mL standard, prepare standard curve dilution as described in the table.

Num.	Standard Volume	Extraction Buffer Volume (µL)	Concentration (µmol/mL)
Std.1	5 µL 500 µmol/mL	995	2.5
Std.2	100 µL of Std.1 (2.5 µmol/mL)	100	1.25
Std.3	100 µL of Std.2 (1.25 µmol/mL)	100	0.625
Std.4	100 µL of Std.3 (0.625 µmol/mL)	100	0.313
Std.5	100 µL of Std.4 (0.313 µmol/mL)	100	0.156
Std.6	100 µL of Std.5 (0.156 µmol/mL)	100	0.078
Std.7	100 µL of Std.6 (0.078 µmol/mL)	100	0.039
Blank	0	100	0

Sample Preparation

Note: We recommend that you use fresh samples. If not assayed immediately, samples can be stored at -80°C for one month.

Add extraction buffer according to the ratio of plant sample mass (g): Extraction Buffer volume (mL) of 1:5-10 (It is recommended to weigh about 0.1 g plant sample and add 1 mL of Extraction Buffer volume). Homogenize at room temperature, centrifuge at 10,000 g for 10 min at 4°C, and keep the supernatant for test.

Assay Procedure

1. Preheat the microplate reader or visible spectrophotometer for more than 30 min, and adjust the wavelength to 625 nm, visible spectrophotometer was returned to zero with deionized water.

2. Operation table (The following were operated in the 96-well plate or microglass cuvette):

Reagent	Blank Well (µL)	Standard Well (µL)	Test Well (µL)
Supernatant	0	0	20
Extraction Buffer	20	0	0
Standard	0	20	0
Reagent I	80	80	80
Reagent II	80	80	80

Mix thoroughly and keep at 25°C for 1 h

Reagent III	20	20	20
-------------	----	----	----

3. After thorough mixing, measure the absorbance value at 625 nm immediately, record it as A_{Blank} , A_{Standard} and A_{Test} . Calculate

$$\Delta A_{\text{Test}} = A_{\text{Test}} - A_{\text{Blank}}, \Delta A_{\text{Standard}} = A_{\text{Standard}} - A_{\text{Blank}}$$

Note: Blank well and standard well only need to measure 1 time. In order to guarantee the accuracy of experimental

results, pre-experiment for 2-3 samples with potential significant difference was recommended.

Data Analysis

Note: We provide you with calculation formulae, including the derivation process and final formula. The two are exactly equal. It is suggested that the concise calculation formula in bold is final formula.

1. Drawing of standard curve:

With the concentration of the standard solution as the x-axis and the $\Delta A_{\text{Standard}}$ as the y-axis, draw the standard curve, get the standard equation $y=kx+b$, and bring the ΔA_{Test} into the equation to get the x value ($\mu\text{mol/mL}$).

2. Calculation of ammonium nitrogen content:

Ammonium nitrogen content ($\mu\text{g/g}$ fresh weight) = $x \times V_{\text{Total sample}} \times 18 \div W = \mathbf{180 \times x}$

$V_{\text{Total sample}}$: added Extraction Buffer volume, 1 mL; W: sample weight, 0.1 g; 18: molar mass of NH_4^+ , $\mu\text{g}/\mu\text{mol}$.

Typical Data

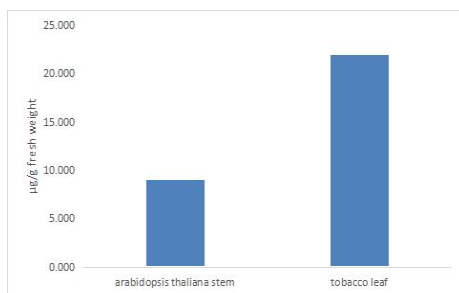


Figure 1. Determination ammonium nitrogen in plant samples by this assay kit

Precautions

1. Protective measures shall be taken during operation.

Recommended Products

Catalog No.	Product Name
KTB3080	CheKine™ Micro Plant Nitrate Nitrogen Assay Kit
KTB1540	CheKine™ Micro Plant Total Phenols (TP) Assay Kit

Disclaimer

The reagent is only used in the field of scientific research, not suitable for clinical diagnosis or other purposes.